

**KAMIYA BIOMEDICAL COMPANY**

# Sheep IgA ELISA

**For the quantitative determination of IgA in sheep serum and plasma**

**Cat. No. KT-1118**

**For Research Use Only.**

## PRODUCT INFORMATION

### **Sheep IgA ELISA** **Cat. No. KT-1118**

#### **PRODUCT**

The **K-ASSAY®** Sheep IgA ELISA is an enzyme immunoassay for the quantitative determination of IgA in sheep serum and plasma. For research use only.

#### **INTRODUCTION**

This ELISA kit is designed for measurement of IgA in sheep serum and plasma. The assay uses rabbit anti-sheep IgA for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated rabbit anti-sheep IgA for detection. Both capture and detection antibodies react specifically with IgA. Cross-reactivity with immunoglobulins from other species has not been investigated.

#### **PRINCIPLE**

Test samples are diluted and incubated in the microtiter wells for 45 minutes alongside sheep IgA calibrators. The microtiter wells are subsequently washed and HRP conjugate is added and incubated for 45 minutes. IgA molecules are thus sandwiched between the immobilization and detection antibodies. After washing the wells to remove unbound HRP-conjugate, TMB reagent is added and incubated for 20 minutes. This results in the development of a blue color. Color development is stopped by the addition of Stop solution; changing the color to yellow. Optical density is measured at 450 nm. The concentration of IgA is proportional to the optical density of the test sample and is derived from a calibration curve.

#### **COMPONENTS**

- Anti sheep IgA coated 96-well plate **Store ≤ -20 °C**
- HRP conjugate stock, 50 µL **Store ≤ -20 °C**
- Sheep IgA stock (lyophilized), 3 vials **Store ≤ -20 °C**
- 20x Wash solution, 50 mL
- Diluent, 50 mL
- TMB reagent, 11 mL
- Stop solution (1N HCl), 11 mL

#### **MATERIALS REQUIRED BUT NOT PROVIDED**

- Distilled or de-ionized water
- Precision pipettes and tips
- Plate reader with an OD range of 0-4 at 450 nm
- Vortex mixer
- Absorbent paper or paper towels
- PC graphing software or graph paper
- Polypropylene or glass tubes
- Plate washer
- Micro-plate incubator/shaker

#### **STORAGE**

The test kit will remain stable for six months from the date of purchase provided that the components are stored appropriately. Store the 96-well plate, IgA stock and HRP conjugate stock vials at or below -20 °C. Store the remaining components in the refrigerator at 4 °C. The microtiter plate should always be kept in a sealed bag with desiccant.

#### **WASH SOLUTION PREPARATION**

The wash solution is provided as a 20X stock. Prior to use, dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water.

## CALIBRATOR PREPARATION

1. Reconstitute the sheep IgA stock as detailed on the vial label. Vortex or mix to ensure complete reconstitution. ***The reconstituted calibrator is stable at 4°C for at least one day but should be aliquoted and frozen at -20°C after reconstitution if future use is intended.***
2. Label 6 polypropylene or glass tubes as 5, 2.5, 1.25, 0.625, 0.313 and 0.156 µg/mL.
3. Into the tube labeled 5 µg/mL, pipette the volume of diluent detailed on the IgA stock vial label. Then add the indicated volume of IgA stock and mix gently. This provides the 5 µg/mL calibrator.
4. Dispense 250 µL of diluent into the tubes labeled 2.5, 1.25, 0.625, 0.313 and 0.156 µg/mL.
5. Prepare a 2.5 µg/mL calibrator by diluting and mixing 250 µL of the 5 µg/mL calibrator with 250 µL of diluent in the tube labeled 2.5 µg/mL.
6. Similarly prepare the remaining calibrators by serial dilution.

## SAMPLE PREPARATION

We found that IgA is present in normal sheep serum at concentrations of ~4 mg/mL. In order to obtain values within range of the calibration curve we suggest that samples initially be diluted 2,000 fold. This can be accomplished using the following procedure for each sample to be tested.

1. Dispense 195 µL and 245 µL of 1x diluent into separate micro centrifuge tubes.
2. Add 5 µL of serum or plasma to the tube containing 195 µL of 1x diluent and gently mix. This provides a 40-fold dilution of the sample.
3. Add 5 µL of the 40-fold diluted sample to the tube containing 245 µL of 1x diluent and gently mix. This provides a 2,000 fold dilution of the sample.

## HRP CONJUGATE PREPARATION

The HRP conjugate should be prepared approximately five minutes before required. The HRP conjugate stock should be diluted with diluent as detailed on the stock vial label.

## ASSAY PROCEDURE

1. Secure the desired number of 8-well strips in the cassette. Store unused strips at -20°C in a sealed plastic bag with desiccant.
2. Dispense 100 µL of calibrators and diluted samples into the wells (we recommend that calibrators and samples be tested in duplicate).
3. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 45 minutes.
4. Aspirate the contents of the microtiter wells and wash the wells 5 times with 1x wash solution using a plate washer (400 µL/well). The entire wash procedure should be performed as quickly as possible.
5. Strike the wells sharply onto adsorbent paper or paper towels to remove residual wash buffer.
6. Add 100 µL of diluted HRP conjugate into each well.
7. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 45 minutes.
8. Wash as detailed in steps 4 to 5 above.
9. Dispense 100 µL of TMB reagent into each well.
10. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 20 minutes.
11. Stop the reaction by adding 100 µL of Stop Solution to each well.
12. Gently mix. *It is important to make sure that all the blue color changes to yellow.*
13. Read the optical density at 450 nm with a microtiter plate reader within 5 minutes.


## CALCULATION OF RESULTS

1. Calculate the average absorbance values ( $A_{450}$ ) for each set of reference calibrators and samples.
2. Construct a calibration curve by plotting the mean absorbance obtained for each reference calibrator against its concentration on linear graph paper, with absorbance on the vertical or Y-axis and concentrations on the horizontal or X-axis.
3. Using the mean absorbance value for each sample, determine the corresponding concentration of IgA from the calibration curve.
4. Multiply the derived concentration by the dilution factor to determine the actual concentration of IgA in the sample.
5. PC graphing software should be used for the above steps if available. We recommend a fit using a second order polynomial equation or a single site, total and nonspecific binding equation.
6. If the  $A_{450}$  values of samples fall outside the calibration curve, samples should be diluted appropriately and re-tested.

## TYPICAL CALIBRATION CURVE

A typical calibration curve with optical density readings at 450 nm on the Y-axis against IgA concentrations on the X-axis is shown below. This curve is for the purpose of illustration only and should not be used to calculate unknowns. A calibration curve should be generated in each experiment.

IgA ( $\mu\text{g/mL}$ )	$A_{450}$
5	2.698
2.5	1.371
1.25	0.792
0.625	0.542
0.313	0.378
0.156	0.361

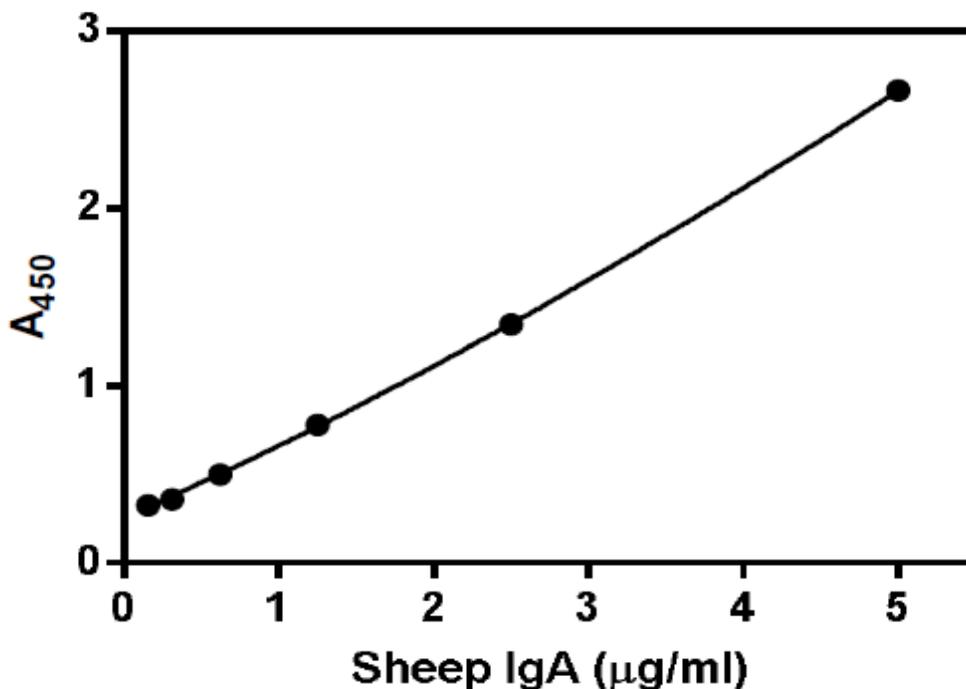

## GENERAL INSTRUCTIONS

1. Please read and understand the instructions thoroughly before using the kit.
2. All reagents except the HRP stock should be allowed to reach room temperature (25 °C) before use.
3. Optimum results are achieved if, at each step, reagents are pipetted into the wells of the microtiter plate within 5 minutes.

## LIMITATIONS OF THE PROCEDURE

1. Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of and in accordance with the instructions detailed above.
2. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.

## FOR RESEARCH USE ONLY

### KAMIYA BIOMEDICAL COMPANY

12790 Gateway Drive, Seattle, WA 98168  
 Tel: (206) 575-8068 Fax: (206) 575-8094  
 Email: LifeScience@k-assay.com  
 www.k-assay.com