

KAMIYA BIOMEDICAL COMPANY

Trout Leukocyte Cell-Derived Chemotaxin 2 (LECT2) ELISA

For the quantitative determination of LECT2 in trout serum

Cat. No. KT-1931

For Research Use Only.

PRODUCT INFORMATION

Trout LECT2 ELISA

Cat. No. KT-1931

PRODUCT

The **K-ASSAY®** Trout LECT2 ELISA is an enzyme immunoassay for the quantitative determination of LECT2 in trout serum. For research use only.

INTRODUCTION

LECT2 (leukocyte cell-derived chemotaxin 2) is a ~16 kDa protein that behaves as a positive acute phase protein in mammals and fish. It was originally identified as a chemotactic factor but also has hepatokine properties. In studies, we found that serum levels of LECT2 increased during bacterial infections.

PRINCIPLE

The assay uses polyclonal antibodies generated against Rainbow Trout LECT2. Horseradish Peroxidase (HRP) conjugated antibodies are used for detection. Calibrators and diluted samples (100 µL) are incubated in the antibody coated microtiter wells for 45 minutes. After washing the wells, HRP-conjugate (100 µL) is added and incubated for 45 minutes. If LECT2 molecules are present, they are sandwiched between the capture and detection antibodies. The wells are then washed to remove unbound HRP-conjugate. TMB is added and incubated for 20 minutes. If LECT2 is present, a blue color develops. Color development is stopped after 20-minutes by addition of Stop Solution, changing the color to yellow. Absorbance is measured at 450 nm. The concentration of LECT2 is proportional to absorbance and is derived from a calibration curve.

COMPONENTS

- Anti-LECT2 coated plate (12 x 8-well strips)
- HRP conjugate stock.
- LECT2 calibrator stock, 2 vials. **Store at -20°C**
- 20x Wash Solution: 50 mL
- Diluent: 2 x 50 mL
- TMB: 11 mL
- Stop Solution: 11 mL

MATERIALS REQUIRED BUT NOT PROVIDED

- Pipettors and tips
- Distilled or de-ionized water
- Polypropylene tubes or 96-well polystyrene plates
- Vortex mixer
- Absorbent paper or paper towels
- Plate incubator/shaker
- Plate washer
- Plate reader capable of measuring absorbance at 450 nm
- Graphing software

GENERAL INSTRUCTIONS

1. All reagents should be allowed to reach room temperature before use.
2. Reliable and reproducible results will be obtained when the assay is conducted with a complete understanding of the instructions and with adherence to good laboratory practice.
3. It is important that calibrators and samples be added to the ELISA plate quickly. If testing large numbers of samples, rather than pipetting calibrators and samples from individual tubes into the ELISA plate, we recommend the following: pipette an excess volume of calibrators and samples into wells of a blank polystyrene 96-well plate. Then use an 8 or 12-channel multi-pipettor to quickly transfer 100 µL aliquots to the wells of the antibody-coated plate.
4. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.

5. Laboratory temperature will influence absorbance readings. The assay was calibrated using a shaking incubator set at 150 rpm and 25°C. Performing the assay at lower temperatures and mixing speeds may result in lower absorbance values.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20X stock. Prior to use, dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water. Unused wash buffer may be stored at 4°C for one week.

DILUENT PREPARATION

The diluent is formulated for measurement of LECT2 in trout and salmon serum or plasma. It is supplied ready to use. DO NOT substitute other buffers.

CALIBRATOR PREPARATION

1. The stock is lyophilized. It is comprised of recombinant Rainbow Trout LECT2 in a stabilizing matrix. Reconstitute it with 200 µL of deionized water, gently mix, and prepare the 25 ng/mL calibrator as described on the vial label.
2. Label seven polypropylene tubes as 12.5, 6.25, 3.13, 1.56, 0.78, 0.39 and 0 ng/mL. Dispense 0.25 mL of diluent into each.
3. Pipette 0.25 mL of the 25 ng/mL LECT2 calibrator into the tube labeled 12.5 ng/mL and mix. This provides the 12.5 ng/mL LECT2 calibrator.
4. Similarly prepare the 6.25 – 0.39 ng/mL calibrators by two-fold serial dilution. If future use is intended, the reconstituted calibrator stock should be stored frozen at or below -20°C within 5 minutes of reconstitution.

HRP CONJUGATE PREPARATION

The HRP conjugate stock must be diluted with diluent as described on the stock vial label about 5 minutes before use. Use 100 µL of the diluted HRP conjugate per well.

SAMPLE PREPARATION

We found LECT2 levels of approximately 1.5 µg/mL in serum from healthy trout. Levels increased to 10 µg/mL or higher three to six days after bacterial infection. To obtain values within range of the calibration curve we found it necessary to dilute trout serum at least 800-fold. Do not test serum at dilutions less than 800-fold because matrix effects may occur. The diluent provided with this kit must be used for dilution. Do not substitute other buffers.

ASSAY PROCEDURE

1. Secure the desired number of 8-well strips in the cassette. Unused strips should be stored in a sealed bag with desiccant at 4°C.
2. Dispense 100 µL of calibrators and samples into appropriate wells. We recommend that calibrators and samples be tested in duplicate.
3. Incubate on a plate shaker at 150 rpm and 25°C for 45 minutes.
4. Empty and wash the microtiter wells 5 times with 1x Wash Solution using a plate washer (400 µL/well).
5. Dispense 100 µL of diluted HRP conjugate into the wells.
6. Incubate on a plate shaker at 150 rpm and 25°C for 45-minutes.
7. Empty and wash the microtiter wells 5 times with 1x Wash Solution using a plate washer (400 µL/well).
8. Strike the wells sharply onto absorbent paper or paper towels to remove all residual droplets.
9. Dispense 100 µL of TMB into each well.
10. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 20 minutes.
11. After 20 minutes stop the reaction by adding 100 µL of Stop Solution to each well.
12. Gently mix. It is important to make sure that all the blue color changes to yellow.
13. Read absorbance at 450 nm with a plate reader within 5 minutes.


CALCULATION OF RESULTS

1. Using curve fitting software, construct a calibration curve by plotting absorbance values of the calibrators versus the LECT2 concentration. We suggest using a second order polynomial (quadratic) equation.
2. Derive the concentration of LECT2 in the samples.
3. Multiply the derived concentration by the dilution factor to determine the concentration in the sample.
4. If the absorbance values of samples fall outside the calibration curve, samples should be diluted appropriately and re-tested

TYPICAL CALIBRATION CURVE


A typical calibration curve is shown below. This curve is for illustration only.

LECT2 (ng/ml)	A ₄₅₀
25	3.567
12.5	1.811
6.25	0.968
3.13	0.589
1.56	0.378
0.78	0.268
0.39	0.228
0	0.144

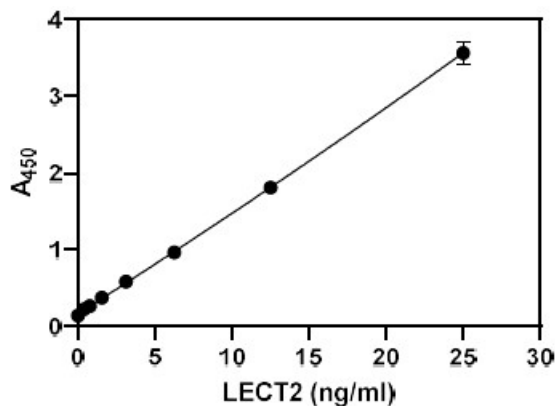

ASSAY PERFORMANCE

Linearity: To assess the linearity of the assay, three Rainbow Trout plasma samples with LECT2 concentrations of 2,270, 3,320, and 6,725 ng/mL were serially diluted to give values within range of the assay.

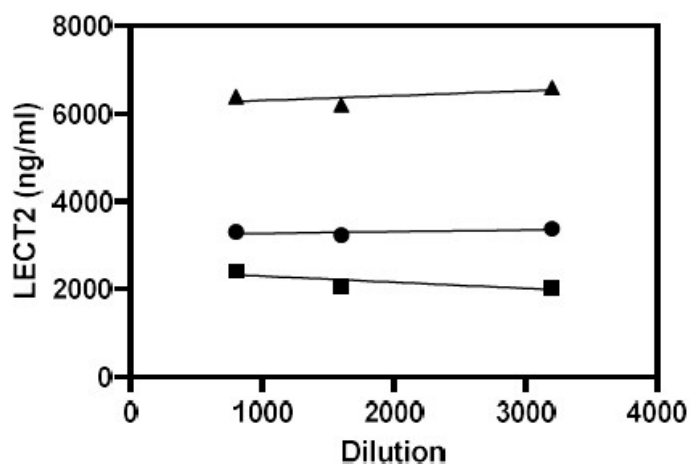

STORAGE

Store the calibrator stock vial at -20°C. The remainder of the kit should be stored at 4°C and the microtiter plate should be kept in a sealed bag with desiccant. The kit will remain stable until the expiration date.

FOR RESEARCH USE ONLY

KAMIYA BIOMEDICAL COMPANY

12779 Gateway Drive, Seattle, WA 98168
 Tel: (206) 575-8068 Fax: (206) 575-8094
 Email: LifeScience@k-assay.com
 www.k-assay.com