

KAMIYA BIOMEDICAL COMPANY

Dog Procalcitonin ELISA

For the quantitative determination of procalcitonin in dog serum

Cat. No. KT-1936

For Research Use Only.

PRODUCT INFORMATION

Dog Procalcitonin ELISA

Cat. No. KT-1936

PRODUCT

The **K-ASSAY®** Dog Procalcitonin ELISA is an enzyme immunoassay for the quantitative determination of procalcitonin in dog serum. For research use only.

INTRODUCTION

Procalcitonin (PCT) is a serum biomarker of bacterial infections and sepsis. In studies, we found levels of approximately 0.5 to 2 ng/mL in healthy dogs. In dogs with infections, we found levels up to 150 ng/mL.

PRINCIPLE

The assay uses two dog PCT antibodies. One is used as coating antibody. The other is conjugated to HRP and used for detection. The calibrator is prepared from recombinant dog PCT. Calibrators and diluted samples (100 µL) are incubated in anti-PCT coated microtiter wells for 45 minutes. After washing the wells, HRP-conjugate (100 µL) is added and incubated for 45 minutes. If PCT molecules are present, they are sandwiched between the capture and detection antibodies. The wells are then washed to remove unbound HRP-conjugate. TMB is added and incubated for 20 minutes. If PCT is present, a blue color develops. Color development is stopped after 20-minutes by addition of Stop Solution, changing the color to yellow. Absorbance is measured at 450 nm. The concentration of PCT is proportional to absorbance and is derived from a calibration curve.

COMPONENTS

- Anti-PCT coated plate (12 x 8-well strips)
- Anti-PCT HRP conjugate, 11 mL
- PCT calibrator stock, 1 vial. **Store at -80°C.**
- 20x Wash Solution: 50 mL
- Diluent: 2 x 50 mL
- TMB: 11 mL
- Stop Solution: 11 mL

MATERIALS REQUIRED BUT NOT PROVIDED

- Pipettors and tips
- Distilled or de-ionized water
- Polypropylene tubes or 96-well polystyrene plates
- Vortex mixer
- Absorbent paper or paper towels
- Plate incubator/shaker
- Plate washer
- Plate reader capable of measuring absorbance at 450 nm
- Graphing software

GENERAL INSTRUCTIONS

1. All reagents should be allowed to reach room temperature before use.
2. It is important that calibrators and samples be added to the ELISA plate quickly. If testing large numbers of samples, rather than pipetting calibrators and samples from individual tubes into the ELISA plate, we recommend the following: pipette an excess volume of calibrators and samples into wells of a blank polystyrene 96-well plate. Then use an 8 or 12-channel multi-pipettor to quickly transfer 100 µL aliquots to the wells of the antibody-coated plate.
3. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.
4. Laboratory temperature will influence absorbance readings. The assay was calibrated using a shaking incubator set at 150 rpm and 25°C. Performing the assay at lower temperatures and mixing speeds may result in lower absorbance values.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20X stock. Prior to use, dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water. Unused wash buffer may be stored at 4°C for one week.

DILUENT PREPARATION

The diluent is formulated for measurement of PCT in serum. It is supplied ready to use. DO NOT substitute other reagents.

CALIBRATOR PREPARATION

1. The calibrator stock is provided as a frozen liquid. Thaw the stock at room temperature a few minutes before preparing the working calibrators. Return the stock to a -80°C freezer immediately after use. It is comprised of pure PCT in a stabilizing matrix.

2. Prepare the 25 ng/mL calibrator as described on the stock vial label.

3. Label seven polypropylene tubes as 12.5, 6.25, 3.13, 1.56, 0.78, 0.39 and 0 ng/mL. Dispense 0.25 mL of diluent into each.

4. Pipette 0.25 mL of the 25 ng/mL PCT calibrator into the tube labeled 12.5 ng/mL and mix. This provides the 12.5 ng/mL PCT calibrator.

5. Similarly prepare the 6.25 to 0.39 ng/mL calibrators by two-fold serial dilution.

SAMPLE PREPARATION

The assay is intended for measurement of PCT in dog serum. In serum from sick dogs, we found PCT levels up to 150 ng/mL. We recommend testing serum at a dilution of 10-fold, but optimal dilutions should be determined by the end user. To avoid matrix effects, do not use dilutions lower than 10-fold. Diluent included with kit must be used for sample dilution.

HRP CONJUGATE PREPARATION

The HRP conjugate is provided as a concentrated stock. Dilution instructions are listed on the vial label. Diluent included with kit must be used for dilution. Use 100 µL per well.

ASSAY PROCEDURE

1. Secure the desired number of 8-well strips in the cassette. Unused strips should be stored in a sealed bag with desiccant at 4°C.

2. Dispense 100 µL of calibrators and diluted samples into appropriate wells. We recommend that calibrators and samples be tested in duplicate.

3. Incubate on a plate shaker at 150 rpm and 25°C for 45 minutes.

4. Empty and wash the microtiter wells 5 times with 1x Wash Solution using a plate washer (400 µL/well).

5. Dispense 100 µL of diluted HRP conjugate into the wells.

6. Incubate on a plate shaker at 150 rpm and 25°C for 45-minutes.

7. Empty and wash the microtiter wells 5 times with 1x Wash Solution using a plate washer (400 µL/well).

8. If necessary, strike the wells sharply onto absorbent paper or paper towels to remove all residual droplets.

9. Dispense 100 µL of TMB into each well.

10. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 20 minutes.

11. After 20 minutes stop the reaction by adding 100 µL of Stop Solution to each well.

12. Gently mix. It is important to make sure that all the blue color changes to yellow.

13. Read absorbance at 450 nm with a plate reader within 5 minutes.

CALCULATION OF RESULTS

1. Using curve fitting software, construct a calibration curve by plotting absorbance values of the calibrators versus the PCT concentration. We suggest fitting data to a second order polynomial equation.


2. Derive the concentration of PCT in the samples and multiply by the dilution factor to determine the concentration in the original sample.

3. If the absorbance values of samples fall outside the calibration curve, samples should be diluted appropriately and re-tested

TYPICAL CALIBRATION CURVE


A typical calibration curve is shown below. This curve is for illustration only.

PCT (ng/ml)	A ₄₅₀
25	3.554
12.5	2.357
6.25	1.277
3.13	0.807
1.56	0.504
0.78	0.364
0.39	0.291
0	0.219

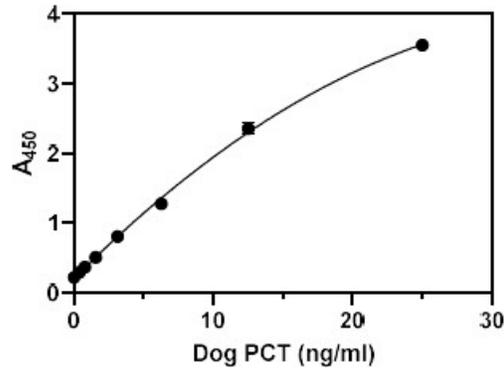

ASSAY PERFORMANCE

Linearity: To assess the linearity of the assay, serum samples with PCT concentrations of 38, 71 and 147 ng/mL were diluted with kit diluent to give values within range of the assay.

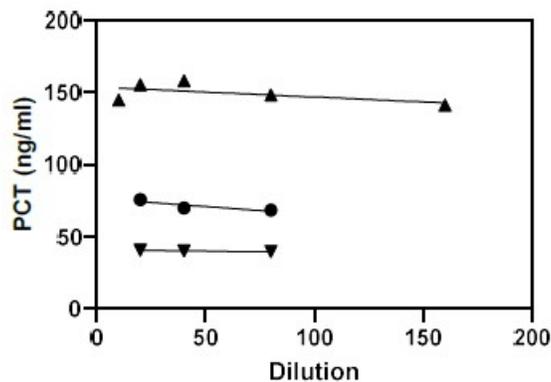

STORAGE

Immediately store the PCT calibrator stock in a -80°C freezer on receipt. The remainder of the kit should be stored at 4°C and the microtiter plate should be kept in a sealed bag with desiccant. The kit will remain stable until the expiration date.

FOR RESEARCH USE ONLY

KAMIYA BIOMEDICAL COMPANY

12779 Gateway Drive, Seattle, WA 98168
 Tel: (206) 575-8068 Fax: (206) 575-8094
 Email: LifeScience@k-assay.com
 www.k-assay.com