



KAMIYA BIOMEDICAL COMPANY

Goat IgM ELISA

For the quantitative determination of IgM in goat serum and plasma

Cat. No. KT-802

For Research Use Only.

PRODUCT INFORMATION

Goat IgM ELISA **Cat. No. KT-802**

PRODUCT

The **K-ASSAY®** Goat IgM ELISA is an enzyme immunoassay for the quantitative determination of IgM in goat serum and plasma. For research use only.

INTRODUCTION

This ELISA kit is designed for measurement of IgM in goat serum and plasma. The assay uses rabbit anti-goat IgM for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated rabbit anti-goat IgM for detection. Both capture and detection antibodies react specifically with goat IgM. Cross-reactivity with immunoglobulins from other species has not been investigated.

PRINCIPLE

Test samples are diluted and incubated in the microtiter wells for 45 minutes alongside goat IgM calibrators. The microtiter wells are subsequently washed and HRP conjugate is added and incubated for 45 minutes. IgM molecules are thus sandwiched between the immobilization and detection antibodies. After washing the wells to remove unbound HRP-conjugate, TMB reagent is added and incubated for 20 minutes. This results in the development of a blue color. Color development is stopped by the addition of Stop solution; changing the color to yellow. Optical density is measured at 450 nm. The concentration of IgM is proportional to the optical density of the test sample and is derived from a calibration curve.

COMPONENTS

- Anti goat IgM coated 96-well plate (12 x 8-well strips) **Store ≤ -20°C**
- HRP conjugate stock, 50 µL **Store ≤ -20°C**
- Goat IgM stock (lyophilized), 3 vials **Store ≤ -20°C**
- 20x Wash solution, 50 mL
- 10x Diluent, 25 mL
- TMB reagent, 11 mL
- Stop solution, 11 mL

MATERIALS REQUIRED BUT NOT PROVIDED

- Distilled or de-ionized water
- Precision pipettes and tips
- Plate reader with an OD range of 0-4 at 450 nm
- Vortex mixer
- Absorbent paper or paper towels
- PC graphing software or graph paper
- Polypropylene or glass tubes
- Plate washer
- Micro-plate incubator/shaker

STORAGE

The test kit will remain stable until the expiration date provided that the components are stored appropriately. Store the 96-well plate, IgM stock and HRP conjugate stock vials at or below -20°C. Store the remaining components in the refrigerator at 4°C. The microtiter plate should always be kept in a sealed bag with desiccant to minimize exposure to damp air.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20X stock. Prior to use, dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water.

DILUENT PREPARATION

The dilution buffer is provided as a 10X stock. Determine the volume of diluent required for your assay and dilute 1 volume of 10x diluent with 9 volumes of distilled or de-ionized water.

CALIBRATOR PREPARATION

1. Reconstitute the goat IgM stock with 1 mL of de-ionized water. Vortex or mix to ensure complete reconstitution. ***The reconstituted calibrator is stable at 4°C for one day.***
2. Label 5 polypropylene or glass tubes as 200, 100, 50, 25 and 12.5 ng/mL.
3. Into the tube labeled 200 ng/mL, pipette 135.0 μ L of diluent. Then 364.96 μ L of IgM stock and mix gently. This provides the 200 ng/mL calibrator.
4. Dispense 250 μ L of diluent into the tubes labeled 100, 50, 25 and 12.5 ng/mL.
5. Prepare a 100 ng/mL calibrator by diluting and mixing 250 μ L of the 200 ng/mL calibrator with 250 μ L of diluent in the tube labeled 100 ng/mL.
6. Similarly prepare the remaining calibrators by serial dilution.

SAMPLE PREPARATION

We found that IgM is present in normal goat serum at concentrations of ~2.5 mg/mL. In order to obtain values within range of the calibration curve we suggest that samples initially be diluted 25,000-fold using the following procedure.

1. Dispense 498 μ L and 495 μ L of 1x diluent into two tubes.
2. Pipette and mix 2.0 μ L of the sample into the first tube containing 498 μ L of diluent. This provides a 250-fold dilution.
3. Mix 5.0 μ L of the 250-fold diluted sample with the 495 μ L of diluent in the second tube. This provides a 25,000-fold dilution of the sample.

HRP CONJUGATE PREPARATION

The HRP conjugate should be prepared approximately five minutes before required. The HRP conjugate stock should be diluted with diluent. Add 2.0 μ L of conjugate to 1.0 mL of diluent for each 8-well strip.

ASSAY PROCEDURE

1. Secure the desired number of 8-well strips in the cassette. Store unused strips at -20°C in a sealed plastic bag with desiccant.
2. Dispense 100 μ L of calibrators and diluted samples into the wells (we recommend that calibrators and samples be run in duplicate).
3. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 45 minutes.
4. Aspirate the contents of the microtiter wells and wash the wells 5 times with 1x wash solution using a plate washer (400 μ L/well). The entire wash procedure should be performed as quickly as possible.
5. Strike the wells sharply onto adsorbent paper or paper towels to remove residual wash buffer.
6. Add 100 μ L of diluted HRP conjugate into each well.
7. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 45 minutes.
8. Wash as detailed in steps 4 to 5 above.
9. Dispense 100 μ L of TMB reagent into each well.
10. Incubate on an orbital micro-plate shaker at 150 rpm at 25°C for 20 minutes.
11. Stop the reaction by adding 100 μ L of Stop Solution to each well.
12. Gently mix. *It is important to make sure that all the blue color changes to yellow.*
13. Read the optical density at 450 nm with a microtiter plate reader within 5 minutes.

CALCULATION OF RESULTS


1. Calculate the average absorbance values (A_{450}) for each set of reference calibrators and samples.
2. Construct a calibration curve by plotting the mean absorbance obtained for each reference calibrator against its concentration in ng/mL on linear graph paper, with absorbance on the vertical or Y-axis and concentrations on the horizontal or X-axis.
3. Using the mean absorbance value for each sample, determine the corresponding concentration of IgM in ng/mL from the calibration curve.
4. Multiply the derived concentration by the dilution factor to determine the actual concentration of IgM in the sample.
5. PC graphing software should be used for the above steps if available. We recommend a fit using a second order polynomial equation.

6. If the A_{450} values of samples fall outside the calibration curve, samples should be diluted appropriately and re-tested.

TYPICAL CALIBRATION CURVE

A typical calibration curve with optical density readings at 450 nm on the Y-axis against IgM concentrations on the X-axis is shown below. This curve is for the purpose of illustration only and should not be used to calculate unknowns. A calibration curve should be generated in each experiment.

IgM (ng/mL)	A_{450}
200	3.152
100	1.563
50	0.746
25	0.380
12.5	0.257

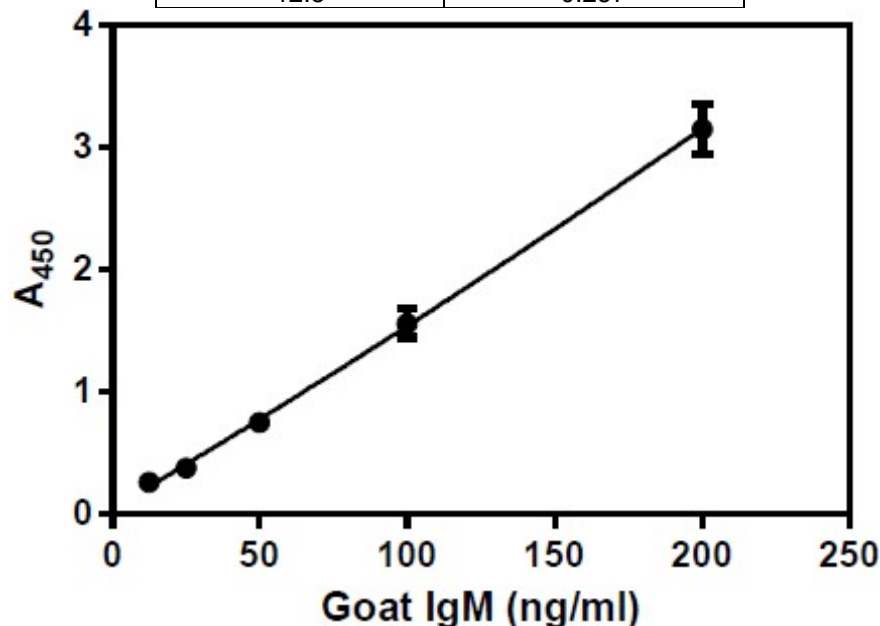

GENERAL INSTRUCTIONS

1. Please read and understand the instructions thoroughly before using the kit.
2. All reagents except the HRP stock should be allowed to reach room temperature (25°C) before use.
3. Optimum results are achieved if, at each step, reagents are pipetted into the wells of the microtiter plate within 5 minutes.

LIMITATIONS OF THE PROCEDURE

1. Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of and in accordance with the instructions detailed above.
2. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.

FOR RESEARCH USE ONLY

KAMIYA BIOMEDICAL COMPANY

12790 Gateway Drive, Seattle, WA 98168
 Tel: (206) 575-8068 Fax: (206) 575-8094
 Email: LifeScience@k-assay.com
 www.k-assay.com