

**KAMIYA BIOMEDICAL COMPANY**

# Goat IgG ELISA

**For the quantitative determination of IgG in goat serum and plasma**

**Cat. No. KT-803**

**For Research Use Only.**

## PRODUCT INFORMATION

### **Goat IgG ELISA** **Cat. No. KT-803**

#### **PRODUCT**

The **K-ASSAY®** Goat IgG ELISA is an enzyme immunoassay for the quantitative determination of IgG in goat serum and plasma. For research use only.

#### **INTRODUCTION**

This ELISA kit is designed for measurement of IgG in goat serum and plasma. The assay uses sheep anti-goat IgG for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated sheep anti-goat IgG for detection. Both capture and detection antibodies react specifically with goat IgG. Cross-reactivity with immunoglobulins from other species has not been investigated.

#### **PRINCIPLE**

Test samples are diluted and incubated in the microtiter wells for 45 minutes alongside goat IgG calibrators. The microtiter wells are subsequently washed and HRP conjugate is added and incubated for 45 minutes. IgG molecules are thus sandwiched between the immobilization and detection antibodies. After washing the wells to remove unbound HRP-conjugate, TMB reagent is added and incubated for 20 minutes. This results in the development of a blue color. Color development is stopped by the addition of Stop solution; changing the color to yellow. Optical density is measured at 450 nm. The concentration of IgG is proportional to the optical density of the test sample and is derived from a calibration curve.

#### **COMPONENTS**

- Anti goat IgG coated 96-well plate **Store ≤ -20°C**
- HRP conjugate stock, 50 µL **Store ≤ -20°C**
- Goat IgG stock (lyophilized), 3 vials **Store ≤ -20°C**
- 20x Wash solution, 50 mL
- 10x Diluent, 25 mL
- TMB reagent, 11 mL
- Stop solution, 11 mL

#### **MATERIALS REQUIRED BUT NOT PROVIDED**

- Distilled or de-ionized water
- Precision pipettes and tips
- Plate reader with an OD range of 0-4 at 450 nm
- Vortex mixer
- Absorbent paper or paper towels
- Curve fitting software
- Polypropylene or glass tubes
- Plate washer
- Micro-plate incubator/shaker

#### **STORAGE**

The kit will remain stable until the expiration date provided that the components are stored appropriately. Store the 96-well plate, IgG stock and HRP conjugate stock vials at or below -20°C. Store the remaining components in the refrigerator at 4°C. The microtiter plate should always be kept in a sealed bag with desiccant to minimize exposure to damp air.

#### **WASH SOLUTION PREPARATION**

The wash solution is provided as a 20X stock. Prior to use, dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water.

## DILUENT PREPARATION

The dilution buffer is provided as a 10X stock. Determine the volume of diluent required for your assay and dilute 1 volume of 10x diluent with 9 volumes of distilled or de-ionized water.

## CALIBRATOR PREPARATION

1. Reconstitute the goat IgG stock with 1 mL of de-ionized water. Vortex or mix to ensure complete reconstitution. ***The reconstituted calibrator is stable at 4°C for one day.***
2. Label 6 polypropylene or glass tubes as 250, 125, 62.5, 31.25, 15.63 and 7.81 ng/mL.
3. Into the tube labeled 250 ng/mL, pipette 404.8  $\mu$ L of diluent. Then add 95.2  $\mu$ L of IgG stock and mix gently. This provides the 250 ng/mL calibrator.
4. Dispense 250  $\mu$ L of diluent into the tubes labeled 125, 62.5, 31.25, 15.63 and 7.81 ng/mL.
5. Prepare a 125 ng/mL calibrator by diluting and mixing 250  $\mu$ L of the 250 ng/mL calibrator with 250  $\mu$ L of diluent in the tube labeled 125 ng/mL.
6. Similarly prepare the remaining calibrators by serial dilution.

## SAMPLE PREPARATION

We found that IgG is present in normal goat serum at concentrations of  $\sim$ 10 mg/mL. In order to obtain values within range of the calibration curve we suggest that samples initially be diluted 150,000-fold using the following procedure.

1. Dispense 998  $\mu$ L and 897  $\mu$ L of 1x diluent into two tubes.
2. Pipette and mix 2.0  $\mu$ L of the sample into the first tube containing 998  $\mu$ L of diluent. This provides a 500-fold dilution.
3. Mix 3.0  $\mu$ L of the 500-fold diluted sample with the 897  $\mu$ L of diluent in the second tube. This provides a 150,000-fold dilution of the sample.

## HRP CONJUGATE PREPARATION

The HRP conjugate should be prepared approximately five minutes before required. The HRP conjugate stock should be diluted with diluent. Add 0.50  $\mu$ L of conjugate to 1.0 mL of diluent for each 8-well strip.

## PROCEDURE

1. Secure the desired number of 8-well strips in the cassette. Store unused strips at  $-20^{\circ}\text{C}$  in a sealed plastic bag with desiccant.
2. Dispense 100  $\mu$ L of calibrators and diluted samples into the wells (we recommend that calibrators and samples be run in duplicate).
3. Incubate on an orbital micro-plate shaker at 150 rpm at  $25^{\circ}\text{C}$  for 45 minutes.
4. Aspirate the contents of the microtiter wells and wash the wells 5 times with 1x wash solution using a plate washer (400  $\mu$ L/well). The entire wash procedure should be performed as quickly as possible.
5. Strike the wells sharply onto adsorbent paper or paper towels to remove residual wash buffer.
6. Add 100  $\mu$ L of diluted HRP conjugate into each well.
7. Incubate on an orbital micro-plate shaker at 150 rpm at  $25^{\circ}\text{C}$  for 45 minutes.
8. Wash as detailed in steps 4 to 5 above.
9. Dispense 100  $\mu$ L of TMB reagent into each well.
10. Incubate on an orbital micro-plate shaker at 150 rpm at  $25^{\circ}\text{C}$  for 20 minutes.
11. Stop the reaction by adding 100  $\mu$ L of Stop Solution to each well.
12. Gently mix. *It is important to make sure that all the blue color changes to yellow.*
13. Read the optical density at 450 nm with a microtiter plate reader within 5 minutes.


## CALCULATION OF RESULTS

1. Using graphing software, construct a calibration curve by plotting the absorbance values of the calibrators versus the  $\log_{10}$  of the IgG concentration and fit the data to a four-parameter logistic equation.
2. Derive the corresponding concentration of IgG in the samples from the calibration curve (remember to derive the concentration from the antilog).
3. Multiply the derived concentration by the dilution factor to determine the actual concentration of IgG in the sample.
4. If the absorbance values of diluted samples fall outside the calibration curve, the original samples should be diluted appropriately and re-tested.

## TYPICAL CALIBRATION CURVE

A typical calibration curve with optical density readings at 450 nm on the Y-axis against IgG concentrations on the X-axis is shown below. This curve is for the purpose of illustration only and should not be used to calculate unknowns. A calibration curve should be generated in each experiment.

IgG (ng/mL)	A <sub>450</sub>
250	2.995
125	2.250
62.5	1.418
31.25	0.693
15.63	0.374
7.81	0.247

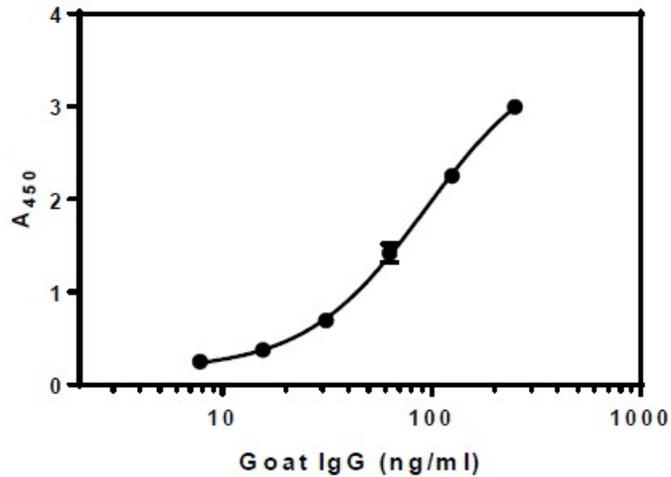

## GENERAL INSTRUCTIONS

1. Please read and understand the instructions thoroughly before using the kit.
2. All reagents except the HRP stock should be allowed to reach room temperature (25°C) before use.
3. Optimum results are achieved if, at each step, reagents are pipetted into the wells of the microtiter plate within 5 minutes.
4. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.

## FOR RESEARCH USE ONLY

### KAMIYA BIOMEDICAL COMPANY

12790 Gateway Drive, Seattle, WA 98168  
 Tel: (206) 575-8068 Fax: (206) 575-8094  
 Email: LifeScience@k-assay.com  
 www.k-assay.com